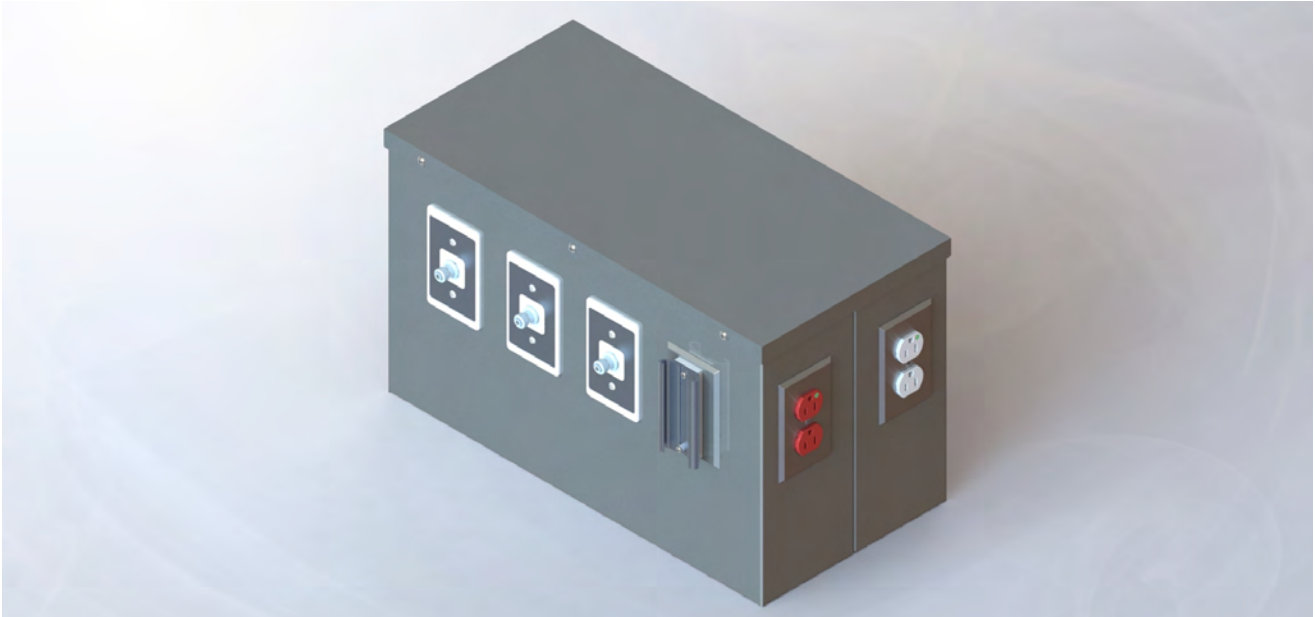


SHADOW series**FLOOR PEDESTAL****Construction Specification**

The Pedestal unit shall consist of a stainless steel shroud forming a 20"(D) x 10"(W) x 12" or 18"(H) rectangular frame. It shall be constructed of 16 gage stainless steel with a number 4 finish and shall have a removable canopy on top for quick access. This product is cULus listed.

Material Specification**Medical Gas**

Medical gas outlets shall be supplied and installed by Medical Design. All outlets to be manifolded on site by local contractor. Installation and testing shall comply with National Fire Protection Association NFPA99 et CSA Z7396.1

Electrical Equipment

Electrical devices shall be furnished pre-installed on the shroud of the pedestal in pre-mounted back box for final site installation. Each devices back box shall be accessible by removing the top access panel. All electrical receptacles are NEMA 5-15/20R, 125 volts AC, hospital grade and comply with CSA and are cULus listed. Receptacles shall be red for emergency and ivory for normal power.

**Electrical wiring and raceway can be provided as an option*

Communication

Communication devices shall be supplied and installed by others. Provisions for devices shall be coordinated with Medical Design.

Shop drawings and submittals

Project specific shop drawings will be produced for every order. Medical Design will manufacture equipment as per signed shop drawings.


Site Installation

Installation of the product includes but is not limited to receiving, storage, erection, clean-up, and waste disposal. All units shall be installed in accordance with Medical Design's installation instructions. The mechanical and electrical contractor shall provide the final connection to the hospital system. The contractor has the responsibility to ensure that every unit complies with all National, State and Local Codes. The contractor shall supply all necessary installation material.

Warranty

Medical Design warrants its architectural products to be free from defects in material and workmanship for a period of twelve (12) months from the date of install. Within this period, Medical Design will repair or replace any part on site, or at the factory, which is proven to be defective at Medical Design's cost.

Furthermore, Medical Design will warrant its material to be free from defect for an additional period of four (4) years [five (5) years from date of install]. Within this period, Medical Design will replace any part, at no charge, which is proven to be defective. Shipping and Installation costs after the first twelve (12) months will be borne by the customer.

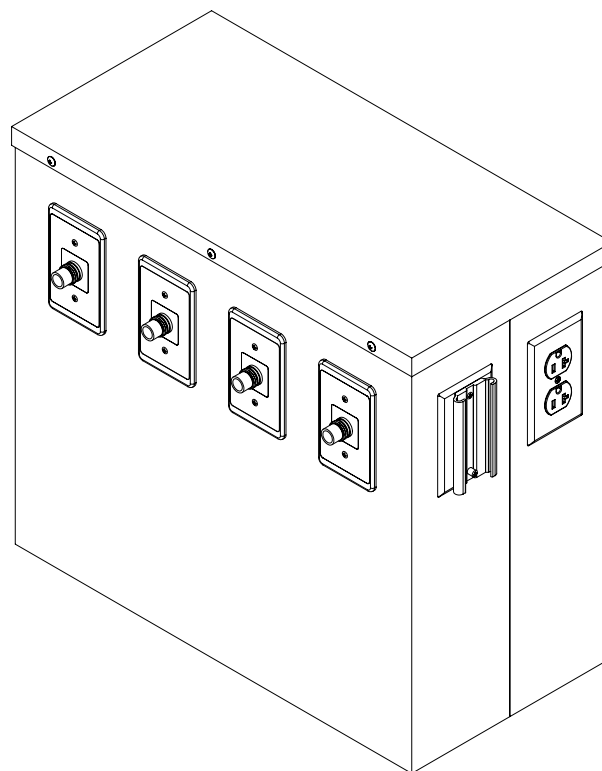

Item number definition

PU-101

Standard Size:

Depth: 20"




Width: 10"

Height: 12" or 18"

SHADOW SERIES FLOOR PEDESTAL

NOTES:

1. ELECTRICAL WIRING TO DEVICES IS TO BE PROVIDED BY OTHERS DURING INSTALLATION OF THE UNIT.
2. MEDICAL GAS OUTLETS INCLUDE PIGTAILS ONLY FOR CONNECTION BY OTHERS (SERVICES ENTER FROM FLOOR BELOW).
3. THE UNIT MUST BE BOLTED TO THE FLOOR USING ADEQUATE ANCHORING DEVICES (BY OTHERS).

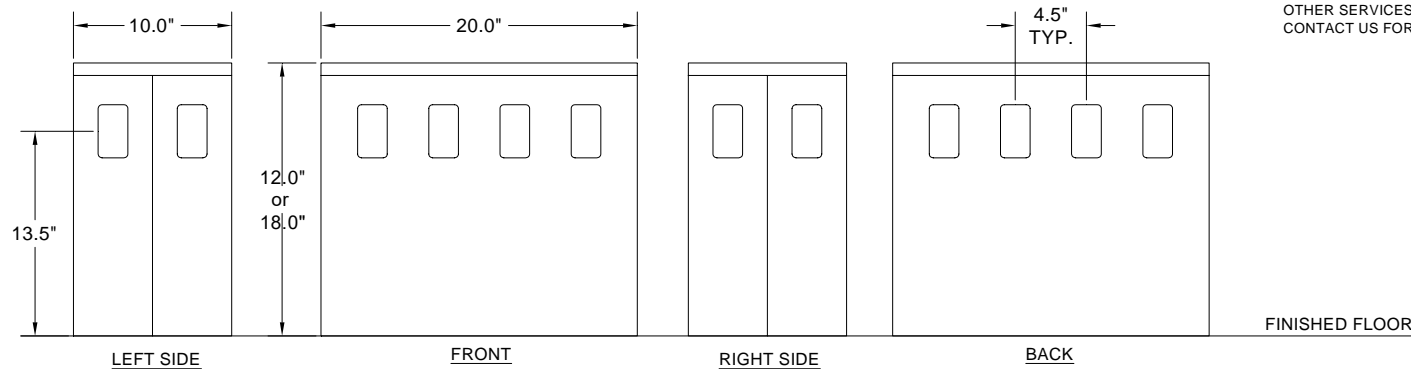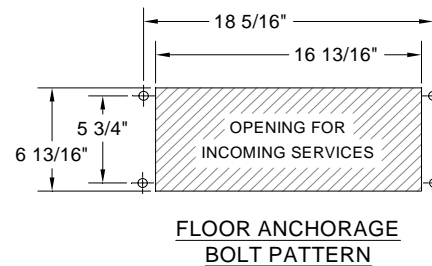

LEGEND

MEDICAL GAS		
ID	QTY	DESCRIPTION
O ₂	-	OXYGEN OUTLET ; Q.C. <input type="checkbox"/> OU D.I.S.S. <input type="checkbox"/>
A	-	MEDICAL AIR OUTLET ; Q.C. <input type="checkbox"/> OU D.I.S.S. <input type="checkbox"/>
V	-	VACUUM OUTLET ; Q.C. <input type="checkbox"/> OU D.I.S.S. <input type="checkbox"/>
N ₂	-	NITROGEN OUTLET ; D.I.S.S. ONLY <input type="checkbox"/>
N ₂ O	-	NITROUS OXIDE OUTLET ; Q.C. <input type="checkbox"/> OU D.I.S.S. <input type="checkbox"/>
EVAC	-	EVACUATION OUTLET ; Q.C. <input type="checkbox"/> OU D.I.S.S. <input type="checkbox"/>
CO ₂	-	CARBON DIOXIDE OUTLET ; D.I.S.S. ONLY <input type="checkbox"/>
ELECTRICITY AND COMMUNICATION		
DR	-	DUPLEX RECEPTACLE, 20A, 125V, H.G., (RED) EMERGENCY POWER (HUBBELL #8300HR)
DW	-	DUPLEX RECEPTACLE, 20A, 125V, H.G., (WHITE) NORMAL POWER (HUBBELL #8300HW)
SR	-	SIMPLEX RECEPTACLE, 20A, 125V, H.G., (RED) EMERGENCY POWER (HUBBELL #8310R)
SW	-	SIMPLEX RECEPTACLE, 20A, 125V, H.G., (WHITE) NORMAL POWER (HUBBELL #8310W)
D	-	DATA PROVISION, 1 GANG
T	-	TELEPHONE PROVISION, 1GANG
B	-	BLANK FACEPLATE, 1 GANG, STAINLESS STEEL
ACCESSORIES		
SL	-	VACUUM BOTTLE SLIDE

OTHER SERVICES AND ACCESSORIES ARE AVAILABLE. CONTACT US FOR MORE INFORMATION.

Hospital Facility Services 612.272.2998 info@hospitalFS.com
*Please contact us for custom designs